



Isofield Stellar

400mm (16") Sterile latex
Cleanroom gloves

Last updated **23 Jul 2025**

PRODUCT CODE

REF

10440

SIZE 6.0	1044060	SIZE 8.0	1044080
SIZE 6.5	1044065	SIZE 8.5	1044085
SIZE 7.0	1044070	SIZE 9.0	1044090
SIZE 7.5	1044075	SIZE 10.0	10440100

CE 2797



PRODUCT INFO

Sterile latex Cleanroom gloves
400mm (16") elbow length
Hand-specific
Natural colour
Textured palm & fingers
Beaded cuff
Low endotoxin levels
Gamma irradiation, minimum 25kGy
Sterility Assurance Level 10^{-6}
Food Safe. Complies limits
established under Regulation (EU)
No 10/2011
Protein level less than 50µg/g
Double donnable
IPA resistant ink pouches

CLEANROOM COMPATIBILITY

GMP Grade A cleanroom
GMP Grade B cleanroom
ISO Class 4 cleanroom
ISO Class 5 cleanroom
Class 10 cleanroom
Class 100 cleanroom

QUALITY ASSURANCE

Manufactured in a facility operating
under ISO 9001:2015 quality
management system
Processed in a NEBB certified
ISO Class 5 cleanroom
Physical properties comply with
European medical glove standard
EN 455-2:2015

APPLICATIONS

Aseptic compounding and mixing
Preparation of sterile emulsions
Manufacture of sterile liquid and
lyophilized vials
Filtration, filling, stoppering and
capping of vials

STORAGE & SHELF LIFE

Store in a dry, cool place (<40°C)
away from direct sunlight
Do not expose open cartons to
prolonged direct fluorescent light
Five (5) years from date of
manufacture

PACKAGING

1 pair per inner PE wallet,
1 PE wallet per sealed PE pouch,
10 pouches per double PE bag,
20 sealed PE bags per lined carton
(200 pairs)

PHYSICAL PROPERTIES

THICKNESS, SINGLE WALL	MM*	MILS	TEST METHOD
Finger tip	0.20	7.87	EN 455-2:2015
Palm	0.17	6.69	EN 455-2:2015
Cuff	0.11	4.33	EN 455-2:2015

* +/- 0.02mm

LENGTH	MIN	TYPICAL	TEST METHOD
From tip of middle finger to edge of cuff	390mm	400mm	EN ISO 21420:2020

STRENGTH PROPERTIES	FORCE AT BREAK	TEST METHOD
Throughout shelf life	≥ 9.0 N	EN 455-2:2015

FREEDOM FROM HOLES	PERFORMANCE	TEST METHOD
Acceptable Quality Level (AQL)	0.65 - Level 3 of 3	EN 374-2:2016

CLEANLINESS PROPERTIES


PARTICLES	TYPICAL PARTICLE COUNT	TEST METHOD
≥ 0.5µm (counts/cm²)	< 1200	IENT-RP-CC005.4

EXTRACTABLES (ION)	TYPICAL VALUE (µg/cm²)	TEST METHOD
Fluoride (F)	0.005	IENT-RP-CC005.4
Chloride (Cl)	0.750	IENT-RP-CC005.4
Nitrite (NO ₂)	0.042	IENT-RP-CC005.4
Bromide (Br)	0.043	IENT-RP-CC005.4
Nitrate (NO ₃)	0.410	IENT-RP-CC005.4
Phosphate (PO ₄)	0.044	IENT-RP-CC005.4
Sulphate (SO ₄)	0.120	IENT-RP-CC005.4
Lithium (Li)	0.006	IENT-RP-CC005.4
Sodium (Na)	0.040	IENT-RP-CC005.4
Ammonium (NH ₄)	0.110	IENT-RP-CC005.4
Potassium (K)	0.050	IENT-RP-CC005.4
Calcium (Ca)	0.510	IENT-RP-CC005.4
Magnesium (Mg)	0.010	IENT-RP-CC005.4
Zinc (Zn)	0.536	IENT-RP-CC005.4

* ND = Not Detected

TECHNICAL PROPERTIES

NORM	TEST REFERENCE	EXPLANATION
Chemical innocuousness	EN ISO 21420:2020	Ensures the gloves do not adversely affect the health of the user. The materials present in the gloves must not release substances that are toxic
Sizing & dexterity	EN ISO 21420:2020 and EN ISO 374-2:2019	Determines sizing compliance and glove dexterity
Air leak & water leak	EN ISO 374-2:2019	Assesses the resistance of the glove to penetration
Chemical degradation	EN ISO 374-4:2019	Determines the resistance to degradation by dangerous chemicals
Chemical permeation	EN 16523-1:2015+A1:2018	Determines the resistance of protective glove materials to permeation by potentially hazardous non-gaseous chemicals
Viral penetration	EN 16604:2004	Assesses the resistance of glove materials to penetration by blood-borne pathogens
Endotoxin test	EN 455-3, USP	Specifies requirements for the evaluation of biological safety for gloves
Sterility validation test	EN ISO 11137 Part 2:2015	Specifies requirements for the development, validation and routine control of a radiation sterilization process
EU type certificate	EN ISO 374-1:2016+A1:2018 Type B EN ISO 374-5:2016 EN ISO 374-4:2019	The applicable essential health and safety requirements of Annex II of the PPE Regulation (EU) 2016/425 as a Category III product
UKCA type certificate	EN ISO 374-1:2016+A1:2018 Type B EN ISO 374-5:2016 EN ISO 374-4:2019	The applicable essential health and safety requirements of PPE Regulation (2016/425) as brought into UK law and amended as a Category III product

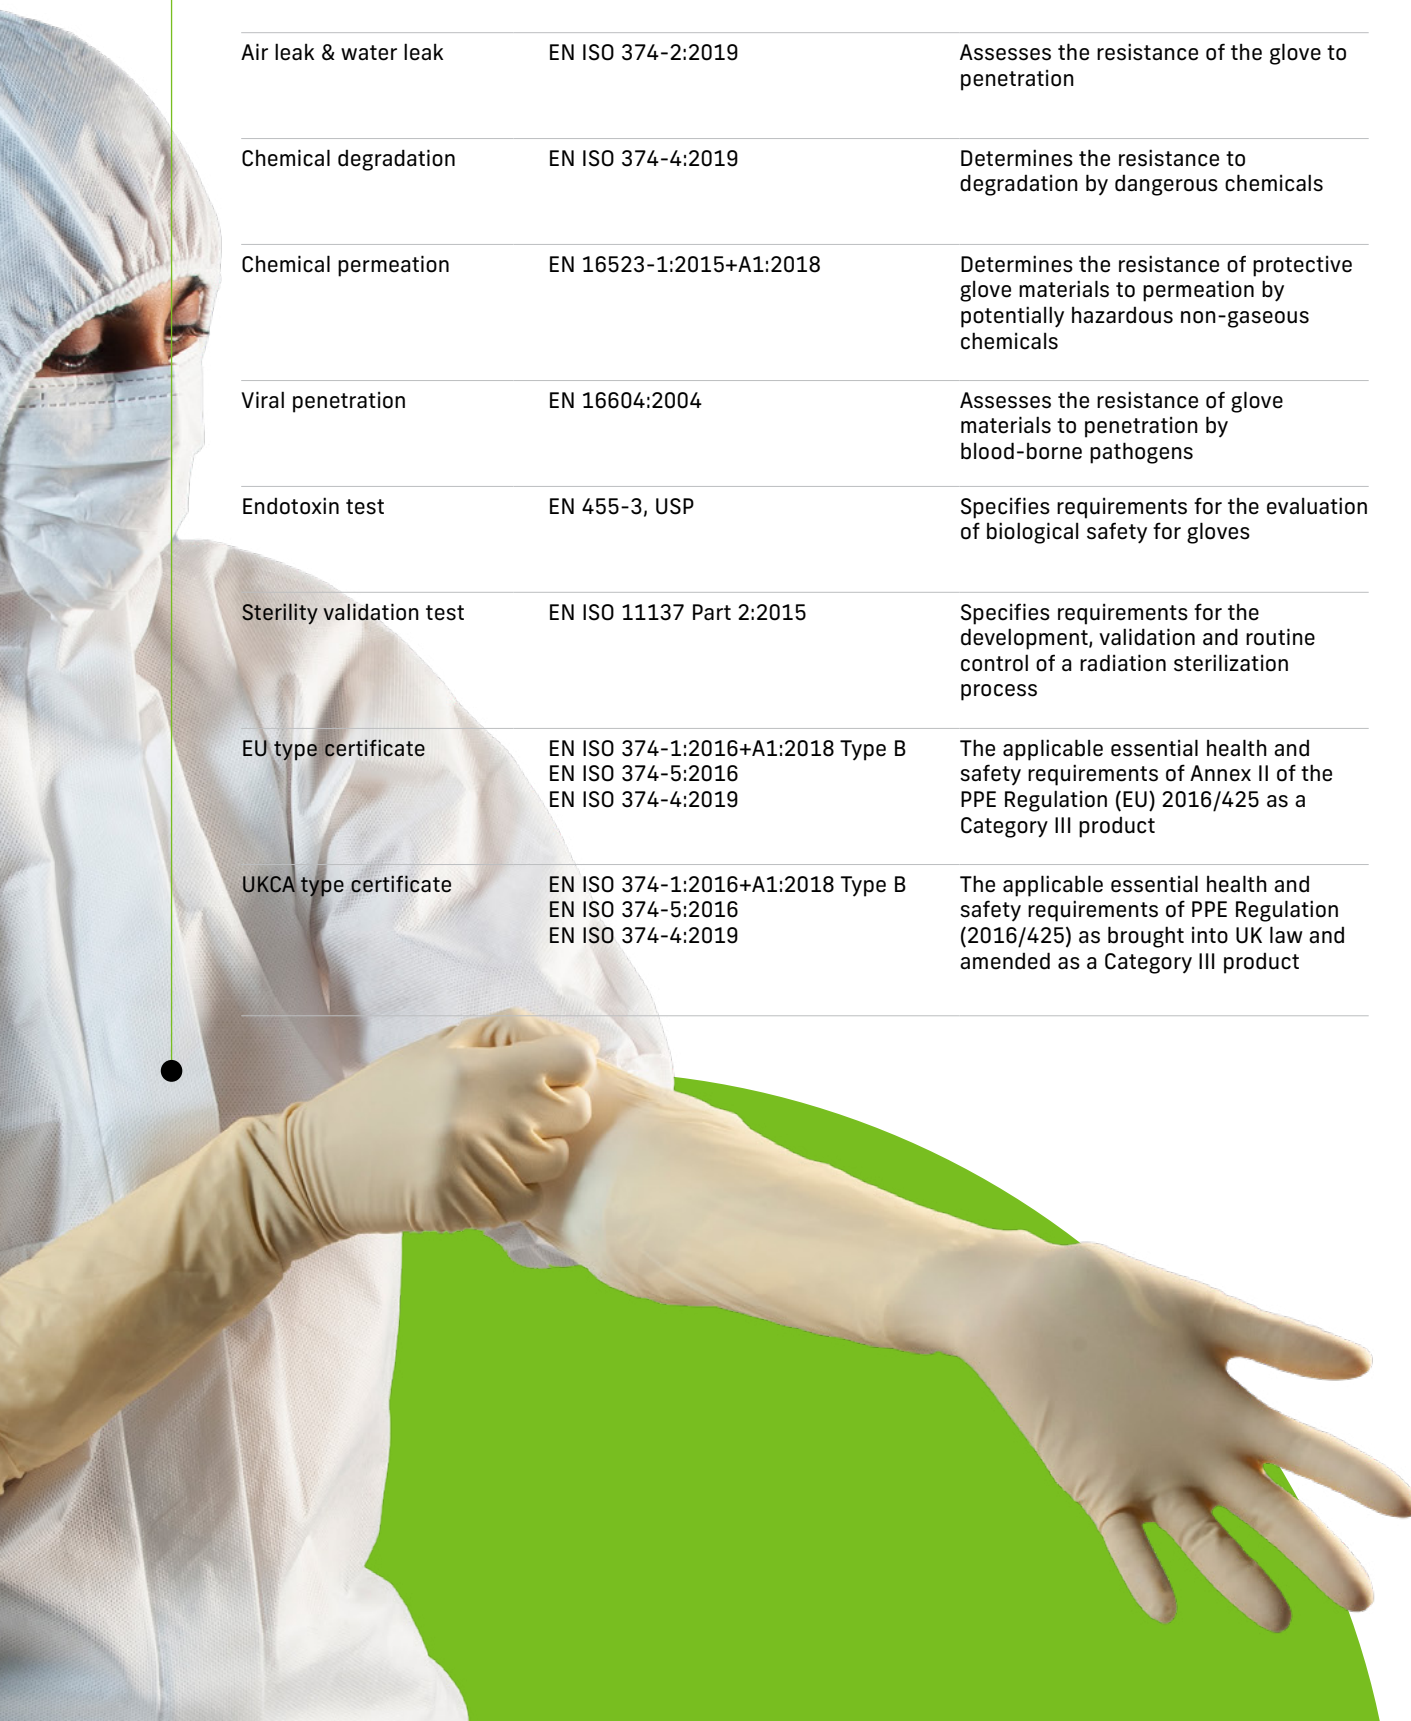

LOADING

	EURO-PALLET	STANDARD PALLET
Pallet size	W80 L120cm	W100 L120cm
Gross weight	9.1 - 10.8kg	9.1 - 10.8kg
Carton size	W28 L32 H37cm	W28 L32 H37cm
Nett weight	6.3 - 8.0kg	6.3 - 8.0kg
Air freight pallet	Max height: 126cm Layers: 3 Cartons: 24	Max height: 126cm Layers: 3 Cartons: 36
Sea freight pallet	Max height: 163cm Layers: 4 Cartons: 32	Max height: 163cm Layers: 4 Cartons: 48

DOCUMENTATION



CERTIFICATE OF CONFORMANCE (COC)
CERTIFICATE OF ANALYSIS (COA)
CERTIFICATE OF IRRADIATION (COI)

please [email us](#)




DECLARATION OF
CONFORMITY (DOC)

[Download](#)



FACTORY RELATED CERTIFICATIONS

To request ISO9001 Certificate,
please [email us](#)

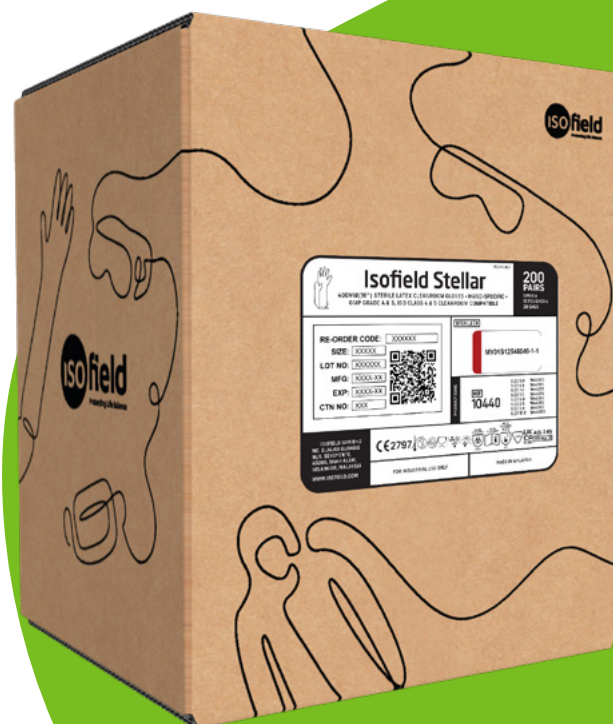

Country of origin: **Malaysia**
HS Code: 4015199000

This data sheet and any other claims made by or on behalf of Isofield shall not be taken as a warranty of merchantability or as a statement that any Isofield products are suitable for a specific purpose. Isofield shall not be held responsible for the end user's choice of product for a particular application.

EUROPE

ISOFIELD (IRELAND) LTD
70 Northumberland Road, Ballsbridge Dublin 4,
Ireland T +44 (0) 1638 6762 39

ASIA

ISOFIELD SDN BHD
6 Jalan Gudang 16/9, Seksyen 16, 40200, Shah Alam,
Selangor, Malaysia, T +603 5512 1709

CONTACT

www.isofield.com
info@isofield.com